SIDECHAIN ANALYTICS

SCAN TO VERIFY
COA-2026-SC-04188
sidechainanalytics.com/verify

CERTIFICATE OF ANALYSIS · BLEND COMPOSITION

bpc157 + tb500

Thymosin β4: 10 mg and BPC-157: 10 mg

Client: **Luxara Research Company - LuxaraLabs.com**

SAMPLE ID **BLD-437_D** ISSUED NOVEMBER 3, 2026

§ 01 Sample Information

Report No.:	**COA-2026-SC-04188**
Lot Number:	**BT2095**
Appearance:	**Lyophilized powder**
Received:	**10/15/2026**
Analyzed:	**11/03/2026**



SAMPLE PHOTOGRAPH

§ 02 Analytical Results

Qualitative and Quantitative chemical analysis by Liquid Chromatography Tandem Mass Spectrometry (HPLC-MS/MS)
Instrument · Agilent 1290 Infinity II with Agilent 6495 QQQ

PEPTIDE	NET CONTENT (mg)	CHROM. PURITY (%)	FILL ACC. (%)
■ Thymosin β4	11.64	99.79	116.4
■ BPC-157	12.10	99.81	121.0
TOTAL NET CONTENT	23.75	—	118.7

BLEND COMPOSITION share of total net peptide content

49% | 51%


DISCLAIMER · RESEARCH USE ONLY

*Results relate **only to the sample as received** by Side-Chain Analytics Inc. and the tests performed, as and when received — not to any other unit, vial, lot, or batch, and not to any other product bearing the same name, label, or description. This report is not a verification of any lot or batch. **For research use only**: this report is not a certificate of quality, safety, efficacy, or regulatory compliance; the material tested is not authorized by Health Canada for human or veterinary use; and this report is not for human or veterinary administration, clinical or diagnostic use, or label claims. Side-Chain Analytics Inc. does not manufacture, source, or sell the material tested and makes **no warranty, express or implied**; its liability shall not exceed the testing fee. This report may not be reproduced except in full, and may not be reproduced, displayed, quoted, or referenced — in whole or in part, including by any badge, seal, or link — in connection with the advertising, offer for sale, sale, or distribution of any product. This certificate is valid only as currently shown at sidechainanalytics.com/verify and may be withdrawn.*


FOR RESEARCH USE ONLY — NOT AUTHORIZED BY HEALTH CANADA FOR HUMAN OR VETERINARY USE

§ 03 Chromatograms

Instrument acquisition — HPLC-MS/MS (MRM). Acquired traces for this sample, labelled by peptide.

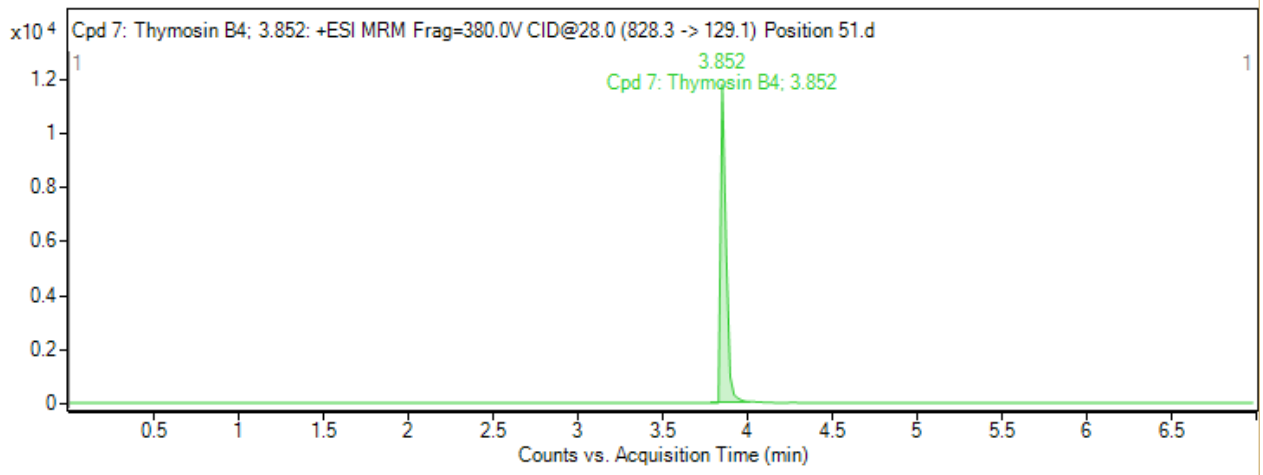

Thymosin β4

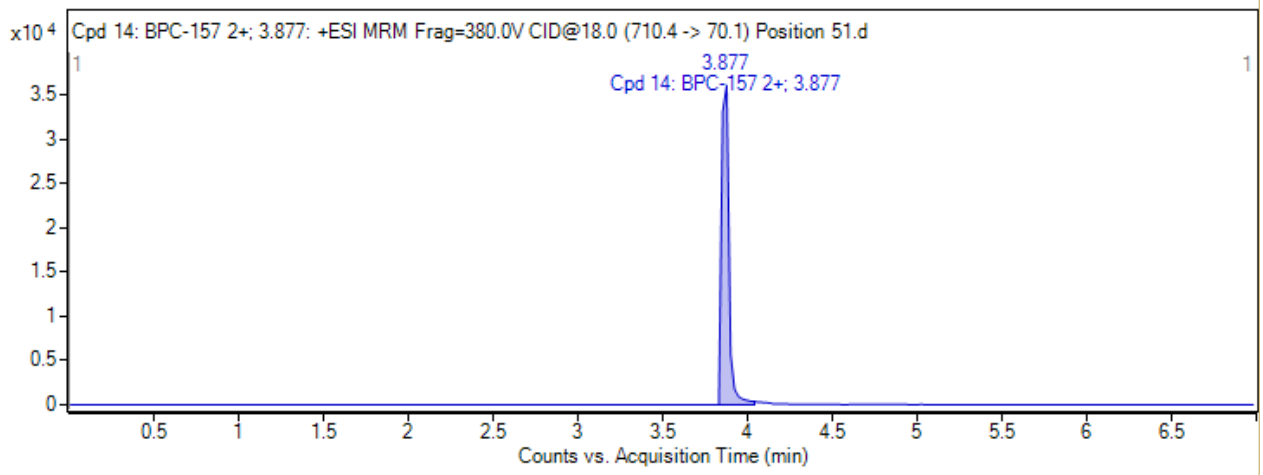

BPC-157